INTERNATIONAL SOCIETY FOR SOIL MECHANICS AND GEOTECHNICAL ENGINEERING

SIMSG   ISSMGE

Foundation conditions analysis for some eolian power units corresponding to the seismic loads influence

Analyse des fondations pour certaines unités d'éoliennes sous chargement sismique

Vintila D., Tenea D.
Ovidius University Constanta, Faculty of civil engineering, Constantza, 900524 Romania

Chirica A.
Technical University of Civil Engineering, Faculty of railways, roads and bridges, Bucharest, 020396 Romania

ABSTRACT: The paper presents the main designing consideration corresponding to some romanian location in order to obtain the most economical foundations. In the eastern part of the Romanian territory (Dobroudgea County) where there are very good wind intensity conditions the geotechnical studies shows the followings three major lithological types: 1. Rocks layer from the top - green schists are at the surface of terrain (0 – 4m deep); 2. Rocks layer is situated between 4m deep to 15m and over it is a lossoidal layer; 3. Rocks layer is deeper then 15m. For each type of soil profile (1,2,3) we have proposed the following foundations: 1. Direct foundation with two variants, as following: a) direct foundation with skirt embeded in green schist, b) direct foundation laying on an improved soil, 2. Pile foundation (embedded in green schist), 3. Floating pile foundation. Paper presents some considerations regarding the influence of seismic loads in foundation design for eolian units.

RÉSUMÉ : L'article présente les aspects principaux afin d'obtenir les fondations les plus économiques dans un site roumain. Dans la partie orientale du territoire roumain (Dobroudja) où il ya de très bonnes conditions d'intensité du vent, les études géotechniques montrent trois types lithologiques principaux: 1. Couche de roches depuis le haut - schistes verts à la surface du terrain (0 - 4 m de profondeur), 2. Couche de roches située entre une profondeur de 4m à 15m et au-dessus couche lossoidale; 3. Couche de roches au-delà de 15m. Pour chaque type de profil de sol (1,2,3), nous avons proposé les fondations suivantes: 1. Fondation directe avec deux variantes, comme suit: a) fondation directe avec jupe encastrée dans le schiste vert, b) fondation posée directement sur un sol amélioré, 2. Fondation sur pieux (intégrés dans le schiste vert), 3. Fondation sur pieux flottants. L'article présente quelques considérations sur l'influence des charges sismiques dans la conception des fondations pour les unités d'éoliennes.

KEYWORDS: eolian power units foundations, seismic loads.

1 INTRODUCTION.

The paper presents the main designing consideration corresponding to some romanian location in order to obtain the most economical foundations for wind farms located in the Eastern part of Romania (Fig. 1, 2).

Because European Union ask that every country from EU has to have at least 20% from its energy generated from renewable sources, Romania prepare itself allowing big wind farms to be located near Black Sea coast in Dobroudgea and beyond Danube in Romanian Plane.

For the moment, usual wind turbines have the following geometrical dimensiones: height – 119m, diameter – 112m, maximum height 175m.

1.1 Seismic conditions

From seismic point of view, Romania has a design code named "*Cod de proiectare seismică – Partea 1, Prevederi de proiectare pentru cladiri P100-2006*". Shear base forces are defined with:

$$F_b = \gamma_I S_d(T_1) m \lambda \quad, \tag{1}$$

where:

γ_I - importance/exposal factor, depending on structure,

$S_d(T_1)$ - response spectrum corresponding to the first period of the structure.

m total weight of structure,

λ correction factor.

As in can be seen in Fig. 1 seismic hazard is described through peak ground acceleration a_g determined for average recurrence interval IMR=50 years for ultimate limite state: $a_g = 0,28$ g ÷ 0,16 g, where g=9,81m/s^2, a_g =2,747 ÷ 1,569 m/s^2.
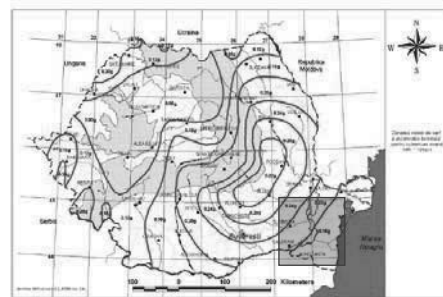

Figure 1 Peak ground acceleration according to P100-2006 and location in Romania.

Figure 2 Corner period according to P100-2006.

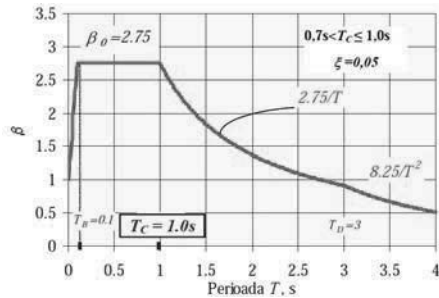Corner period for response spectra for this sites can be Tc=1 s or 0,7s (Fig. 2).

Figure 3 Normalized spectrum for acceleration's elastic response according to P100-2006

From 2012 in Romania is proposed another design code named "*Cod de proiectare seismică – Partea 1, Prevederi de proiectare pentru cladiri P100/1-2012*". Main difference is that it design value of seismic force for is defined for 225 years average recurrence interval (probability of exceeding 20% in 50 years).

As in can be seen in Fig. 4 seismic hazard is described through peak grouns acceleration a_g determined for average recurrence interval IMR=225 years for ultimate limite state a_g = 0,30 g ÷ 0,20 g, where g=9,81m/s^2, a_g =2,943 ÷ 1,962 m/s^2.
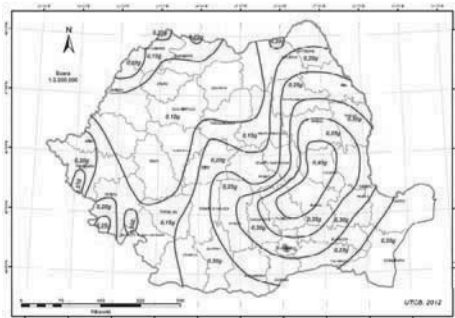

Figure 4 Peak ground acceleration according to P100-2012.

From natural frequencies point of view (Fig. 7) it can be seen that almost every type o wind turbine (with steel or concrete tower) has natural period over 3,2 s, even if the soil is stiff, average or soft.

Figure 5 Corner period according to P100-2012.

Regarding corner period (Fig. 6) the same zones will be used.

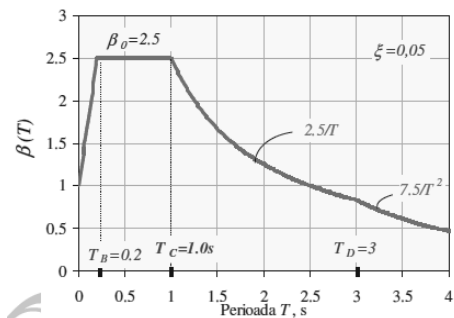Main differences are at $T_B=0,2T_C$, so that $T_B=0,2$ s.

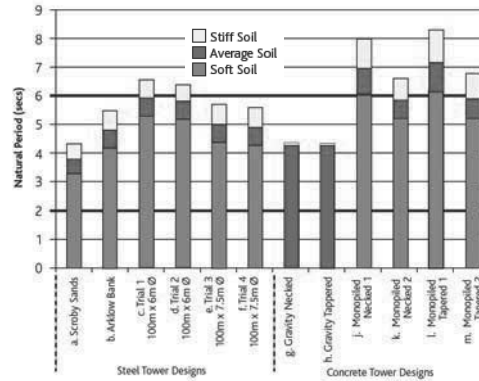Figure 6 Normalized spectrum for acceleration's elastic response according to P100-2012.

Figure 7 Natural periods for WT (Gifford – Concrete towers for Onshore and Offshore wind farms)

2 GEOTECHNICAL INVESTIGATIONS

Geotechnical studies show the followings three major types of lithology:

1. Rocks layer from the top - green schists are at the surface of terrain (0 – 4m deep)
2. Rocks layer is situated between 4m deep to 15m and over it is a leossoidal layer.
3. Rocks layer is deeper than 15m.

Geotechnical investigation were made respecting national standard NP 074/2007. Drillings were made, corresponding to each wind turbine location during November 2011 to march 2012 using WIRTH HD 10S and L100 machines.

First general conclusion of this studies is that a layer of about 25m of dusty sandy clays saturated with low consistency thin intercalations non-cohesive nature is on each site. This is also confirmed in geoelectrical studies.
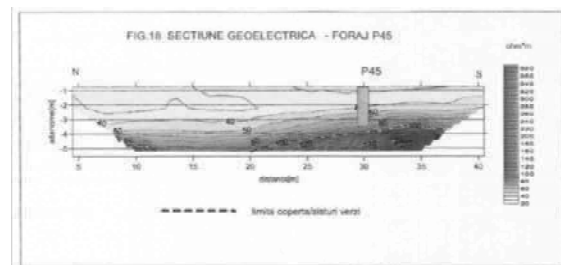

Figure 8 Geoelectrical section through P45.

It is confirmed that resistivities for the first 22m of soil is very low between 1.5 ÷ 5.5 ohm$x$m. From 22m depth resistivities are increasing to values between 25 ÷ 40 ohm$x$m which suggest cohesive lithological formations with better consistency.

For low consistency clays were made also dynamic tests in cyclic triaxial compressive machine and in resonant column.

Compression tests were performed in edometer in order to obtain edometric modulus and unit deformation. The maximum vertical effort of 300kPa was applied to identify stress - strain relationship in compression area (charge) / decompression. In terms of compressibility characteristics of site materials fall into

the category of soil with high compressibility in natural conditions and very high in flooded conditions. M2-3 edometric module and value of unit deformation under normal specific effort level of 200kPa were considered for flooded samples.

In order to study the effect of treatment with (Portland) cement for soft clay samples were also performed compression test-settlement. Samples were treated with 8% and 12% cement were tested in terms of site saturated with salt water after 6 days. An increase in the amount of edometric modulus M2-3 from 4.167 kPa to 5.262 kPa in mixed with 8% cement (20% increase) and 6897 kPa mixed with 12 % cement (60% increase). On samples from drilling were also conducted tests to determine the shear strength parameters, both by direct shear test and triaxial tests. In direct shear apparatus, saturated samples were tested taking into account site conditions (nature-soil and geological effort applied) being sheared in conditions CU (consolidation effort geological area, v = 0.5mm/minut - sheared undrained) and in CD conditions (geological consolidation effort, v = 0.05m/minut - sheared drained).

On undisturbed samples belonging to the main geological formations were performed following types of tests: - Type direct shear tests consolidated - undrained (CU) and consolidated-drained or type (CD); - Compressive load and strain controlled triaxial stress conditions measured anisotropic type CKoD and CKoU, respectively; - Triaxial compression tests with strain imposed and effort to follow those measures pore water pressure variation CKoU;

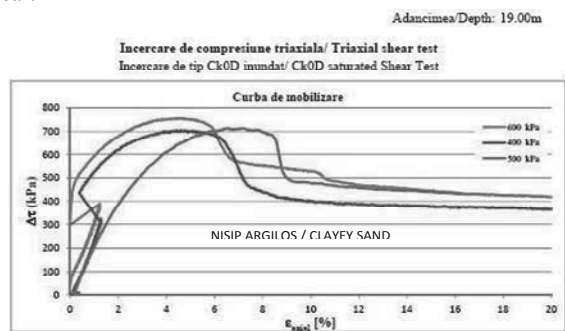Are presented the stress-strain relationships recorded during shear.

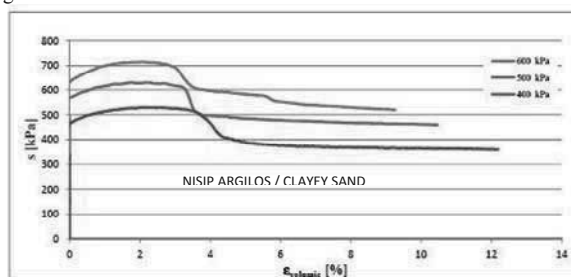Figure 9 Triaxial shear test CK0D - $\Delta\tau$.

Figure 10 Triaxial shear test CK0D - s.

From this analysis some conclusions can be drawn valid for the entire site of the wind farm, namely:

- The mean experimental deformation module where a degree of mobilization of shear strength of 60% are: $E_n = (10 \div 11) \times 10^3$ kPa for clayey sands located at depths of over 20 m; $E_n = (5 \div 6) \times 10^3$ kPa for clay dusts located at depths of over 10 m; $E_n = (6 \div 7) \times 10^3$ kPa for clays located at depths of over 10 m;

Graphic processing geotechnical data field and laboratory investigation is shown in Figure - Correlation lithological column highlighting the systematic sequence.

In cyclic triaxial test machine anisotropic samples were consolidated on effort path k_0. Each sample was tested as follows: in the first stage from a vertical axial displacement imposed to 0.01mm is determined dynamic modulus at different frequencies from 0.5Hz to 2.0Hz, then for the other steps axial

displacement is changed from 0.02mm, 0.05mm, 0.1mm, 0.2mm, 0.5mm, 1.0mm, 1.5mm, 2.0mm, 3.0mm, 4.0mm, 6mm and 8.0mm respectively, keeping the same type of frequencies. Modulus of deformation values in linear dynamic conditions in the analyzed frequency decreases greatly on clay samples saturated soft with plastic strain values.
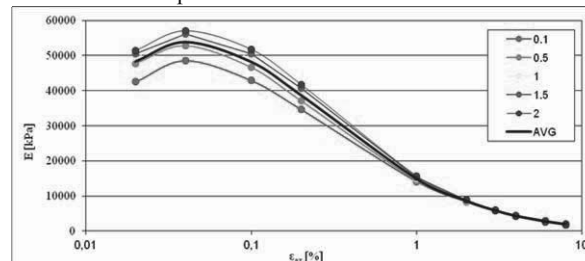

Figure 11 Mobilization curves for G-2, P6 – 15.0m (F2)
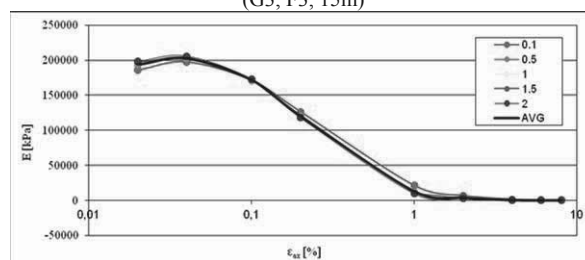
(G3, F3, 15m)

Figure 12 Mobilization curves for G-2, P9 – 22.0m
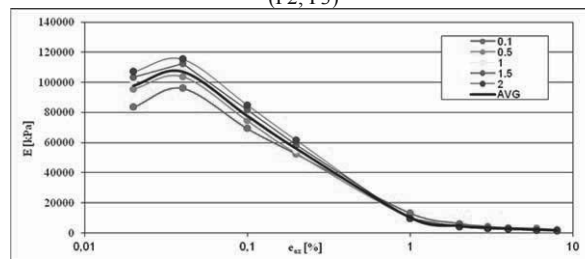
(F2; F3)

Figure 13 Mobilization curves for G-2, P10 – 25.0m (F2)
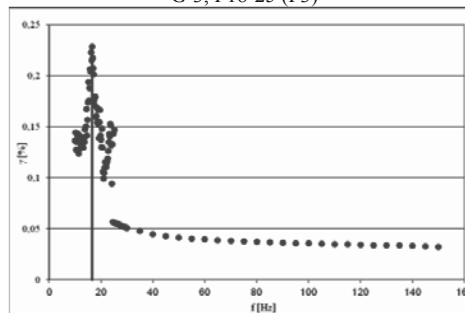
G-3, P18-25 (F3)

Figure 14 Resonant frequency for torsion is 16.6Hz for the sample silty clay G-2, P06 – 15.0m; (F2); G-3 (F3)
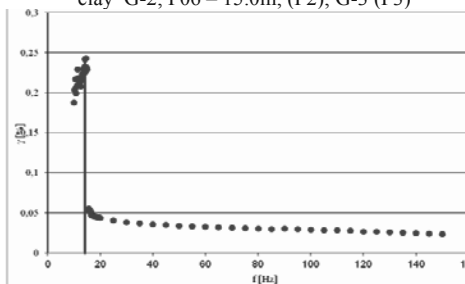

Figure 15 Resonant frequency for flexure is 14.2Hz for the sample clayey silt G-2, P06 – 15.0m, (F3; G3 – F3)

3. CONCLUSIONS

Given the physical and mechanical characteristics of the subsoil in static and dynamic conditions as presented in the previous chapters, 3 types of foundation is recommended for generator:

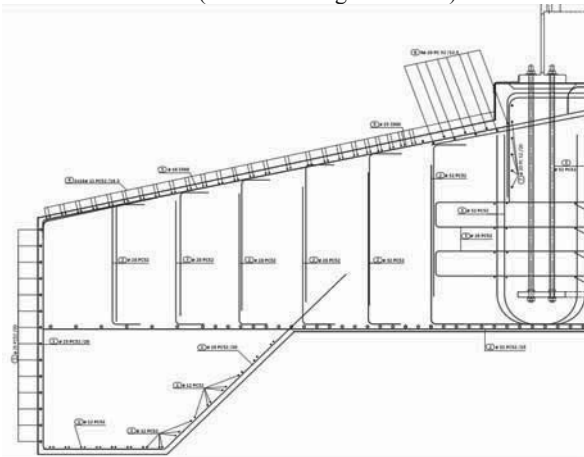1.a Direct foundation (embedded in green schist).

Figure 16 Transversal section of reinforced concrete foundation with skirt.

As it can be seen from the image above, we propose to make at the edge of foundation along its perimeter, a skirt in fact or a so called "fusta" in romanian language. The first reason to do this is to embed the foundation in a rock with good quality, but not on all foundation surface. The second reason is to have a havier foundation on its edges, to prevent it's movement during eartquake. Also this kind of improvement reduce the pressures on soil and increse the active surface from 54% for direct foundation without skirt to 70% for direct foundation with skirt as it can be seen in Fig. 12.

1.b Direct foundation on improved soil (Fig. 18) by methods compatible with saturated soft clay with salt water; the minimum height for slab is 5.00 m, bottom slab will be designed as a rigid compensating box with a "skirt" on outline circular for plastic yielding reduced growth areas and rotation. The wind tower foundation can be optimized by making "slurry" wall with thickness of 80 cm on circular diameter contour ~ 20 m to 20 m depth before land improvement. Also this kind of improvement, reduce the pressures on soil and increase the active surface.
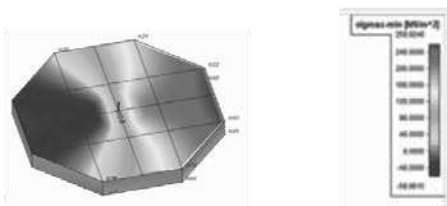

Figure 17 Pressure under foundation with skirt.

a) indirect foundation through a system of piles - large diameter piles connected by a slab designed as a rigid compensating box for reduced deformations.
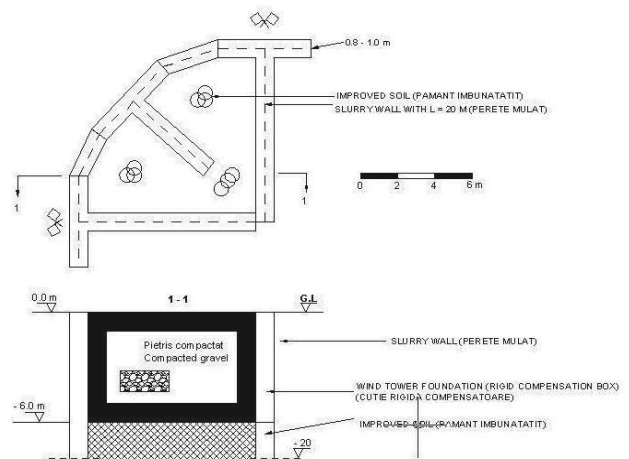b) Mixt foundation: piles foundation on improved soil.

Figure 18 Direct foundation details on improved soil

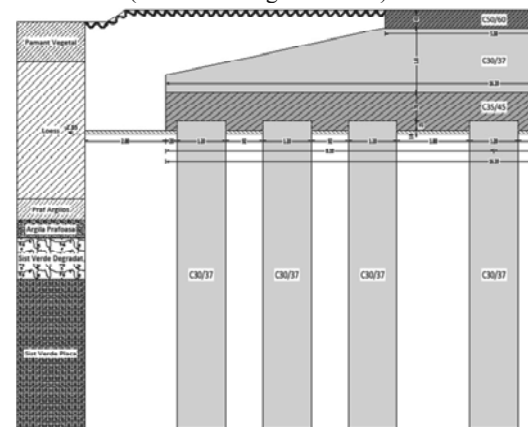2. Pile foundation (embedded in green schist)

Figure 19 Transversal section of pile foundation.

Depending on load case in can be seen that axial forces on pile varies a lot from compressions (+1933,63kN) at left to traction (-9,42kN) at right. Piles for this type of foundations are 1,08 m in diameter reinforced with 26 bars ϕ20 of steel.

3.Floating pile foundation.

For this type of foundation the distribution of piles is the same with no. 2. Total lengh of this piles is more than 24m. This type of foundation is applicable to the situation where loessial soil stratum is greater than 20m.

1 REFERENCES

Indraratna, B.; Chu, J.; Hudson, J.A. [2005] - "*Ground improvement - case histories*", Elsevier Geo-Engineering Book series, volume 3.

Moseley, M. P. & Kirsch, K. [2004] - "*Ground improvement*" 2nd Edition, Taylor & Francis

G. F. Technical Expert S.R.L. – "*Geotechnical study for wind park Surdila – Gaiseanca*", [2012].

Vintila, D., Tenea, D., Chirica, A. [2010] - "*Designing optimization for some eolian power unit taking into account the seismic loads influence*", Fifth International Conference on Recent Advances in Geotechnical Earthquake Engineering and Soil Dynamics, San Diego, California

Chirica, A., Vintila, D., Tenea, D., [2013] - "*Foundations conditions study for aeolian power units on soft soils under static and seismic loads. Case study*", Seventh International Conference on Case histories in Geotechnical Engineering, Chicago.